

(19) World Intellectual Property Organization  
International Bureau(43) International Publication Date  
7 August 2003 (07.08.2003)

PCT

(10) International Publication Number  
WO 03/063735 A2

(51) International Patent Classification: A61F 2/06

(21) International Application Number: PCT/US03/02124

(22) International Filing Date: 22 January 2003 (22.01.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:  
10/066,426 30 January 2002 (30.01.2002) US(63) Related by continuation (CON) or continuation-in-part (CIP) to earlier application:  
US 10/066,426 (CON)  
Filed on 30 January 2002 (30.01.2002)

(71) Applicant (for all designated States except US): CARDIAC DIMENSIONS, INC. [US/US]; 5540 Lake Washington Blvd., Kirkland, WA 98033 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): MATHIS, Mark,

L. [US/US]; 10624 Northeast 60th Street, Kirkland, WA 98033 (US). NIEMINEN, Gregory, D. [US/US]; 20206 - 100th Avenue NE, Bothell, WA 98011 (US). REUTER, David, G. [US/US]; 3225 - 208th PISE, Bothell, WA 98021 (US).


(74) Agents: GRAY, Richard, O., Jr. et al.; Graybeal Jackson Haley LLP, 155 - 108th Avenue NE, Suite 350, Bellevue, WA 98004-5901 (US).

(81) Designated States (national): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, OM, PH, PL, PT, RO, RU, SD, SE, SG, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZM, ZW.

(84) Designated States (regional): ARIPO patent (GL, GM, KH, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, SE, SI,

[Continued on next page]

(54) Title: FIXED LENGTH ANCHOR AND PULL MITRAL VALVE DEVICE AND METHOD

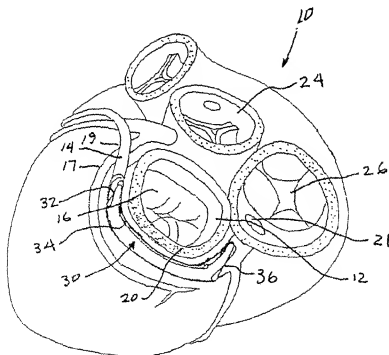

(57) Abstract: A device effects the mitral valve annulus geometry of a heart. The device includes a first anchor configured to be positioned within and anchored to the coronary sinus of the heart adjacent the mitral valve annulus within the heart and a second anchor configured to be positioned within the coronary sinus of the heart proximal to the first anchor and adjacent the mitral valve annulus within the heart. The second anchor, when deployed, anchors against distal movement and is moveable in a proximal direction. The device further includes a connecting member having a fixed length permanently attached to the first and second anchors. As a result, when the first and second anchors are within the coronary sinus with the first anchor anchored in the coronary sinus, the second anchor may be displaced proximally to effect the geometry of the mitral valve annulus and released to maintain the effect on the mitral valve geometry.

WO 03/063735 A2



SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

*For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*

**Published:**

— *without international search report and to be republished upon receipt of that report*

**FIXED LENGTH ANCHOR AND PULL MITRAL VALVE DEVICE AND METHOD***Field of the Invention:*

[1] The present invention generally relates to a device  
5 and method for treating dilated cardiomyopathy of a heart. The  
present invention more particularly relates to a device and  
method for reshaping the mitral valve annulus.

*Background of the Invention:*

10 [2] The human heart generally includes four valves. Of  
these valves, a most critical one is known as the mitral valve.  
The mitral valve is located in the left atrial ventricular  
opening between the left atrium and left ventricle. The mitral  
valve is intended to prevent regurgitation of blood from the  
15 left ventricle into the left atrium when the left ventricle  
contracts. In preventing blood regurgitation the mitral valve  
must be able to withstand considerable back pressure as the left  
ventricle contracts.

[3] The valve cusps of the mitral valve are anchored to  
20 muscular wall of the heart by delicate but strong fibrous cords  
in order to support the cusps during left ventricular  
contraction. In a healthy mitral valve, the geometry of the  
mitral valve ensures that the cusps overlies each other to  
preclude regurgitation of the blood during left ventricular  
25 contraction.

[4] The normal functioning of the mitral valve in  
preventing regurgitation can be impaired by dilated  
cardiomyopathy caused by disease or certain natural defects.  
For example, certain diseases may cause dilation of the mitral  
30 valve annulus. This can result in deformation of the mitral  
valve geometry to cause ineffective closure of the mitral valve  
during left ventricular contraction. Such ineffective closure  
results in leakage through the mitral valve and regurgitation.

Diseases such as bacterial inflammations of the heart or heart failure can cause the aforementioned distortion or dilation of the mitral valve annulus. Needless to say, mitral valve regurgitation must not go uncorrected.

5 [5] One method of repairing a mitral valve having impaired function is to completely replace the valve. This method has been found to be particularly suitable for replacing a mitral valve when one of the cusps has been severely damaged or deformed. While the replacement of the entire valve eliminates  
10 the immediate problem associated with a dilated mitral valve annulus, presently available prosthetic heart valves do not possess the same durability as natural heart valves.

[6] Various other surgical procedures have been developed to correct the deformation of the mitral valve annulus and thus  
15 retain the intact natural heart valve function. These surgical techniques involve repairing the shape of the dilated or deformed valve annulus. Such techniques, generally known as annuloplasty, require surgically restricting the valve annulus to minimize dilation. Here, a prosthesis is typically sutured  
20 about the base of the valve leaflets to reshape the valve annulus and restrict the movement of the valve annulus during the opening and closing of the mitral valve.

[7] Many different types of prostheses have been developed for use in such surgery. In general, prostheses are annular or  
25 partially annular shaped members which fit about the base of the valve annulus. The annular or partially annular shaped members may be formed from a rigid material, such as a metal, or from a flexible material.

[8] While the prior art methods mentioned above have been  
30 able to achieve some success in treating mitral regurgitation, they have not been without problems and potential adverse consequences. For example, these procedures require open heart surgery. Such procedures are expensive, are extremely invasive

requiring considerable recovery time, and pose the concomitant mortality risks associated with such procedures. Moreover, such open heart procedures are particularly stressful on patients with a comprised cardiac condition. Given these factors, such procedures are often reserved as a last resort and hence are employed late in the mitral regurgitation progression. Further, the effectiveness of such procedures is difficult to assess during the procedure and may not be known until a much later time. Hence, the ability to make adjustments to or changes in the prostheses to obtain optimum effectiveness is extremely limited. Later corrections, if made at all, require still another open heart surgery.

[9] An improved therapy to treat mitral regurgitation without resorting to open heart surgery has recently been proposed. This is rendered possible by the realization that the coronary sinus of a heart is near to and at least partially encircles the mitral valve annulus and then extends into a venous system including the great cardiac vein. As used herein, the term "coronary sinus" is meant to refer to not only the coronary sinus itself but in addition, the venous system associated with the coronary sinus including the great cardiac vein. The therapy contemplates the use of a device introduced into the coronary sinus to reshape and advantageously effect the geometry of the mitral valve annulus.

[10] The device includes a resilient member having a cross sectional dimension for being received within the coronary sinus of the heart and a longitudinal dimension having an unstressed arched configuration when placed in the coronary sinus. The device partially encircles and exerts an inward pressure on the mitral valve. The inward pressure constricts the mitral valve annulus, or at least a portion of it, to essentially restore the mitral valve geometry. This promotes effective valve sealing action and eliminates mitral regurgitation.

[11] The device may be implanted in the coronary sinus using only percutaneous techniques similar to the techniques used to implant cardiac leads such as pacemaker leads. One proposed system for implanting the device includes an elongated

5 introducer configured for being releasably coupled to the device. The introducer is preferably flexible to permit it to advance the device into the heart and into the coronary sinus through the coronary sinus ostium. To promote guidance, an elongated sheath is first advanced into the coronary sinus.

10 Then, the device and introducer are moved through a lumen of the sheath until the device is in position within the coronary sinus. Because the device is formed of resilient material, it conforms to the curvatures of the lumen as it is advanced through the sheath. The sheath is then partially retracted to

15 permit the device to assume its unstressed arched configuration. Once the device is properly positioned, the introducer is then decoupled from the device and retracted through the sheath. The procedure is then completed by the retraction of the sheath. As a result, the device is left within the coronary sinus to exert

20 the inward pressure on the mitral valve to restore mitral valve geometry.

[12] The foregoing therapy has many advantages over the traditional open heart surgery approach. Since the device, system and method may be employed in a comparatively noninvasive

25 procedure, mitral valve regurgitation may be treated at an early stage in the mitral regurgitation progression. Further, the device may be placed with relative ease by any minimally invasive cardiologist. Still further, since the heart remains completely intact throughout the procedure, the effectiveness of

30 the procedure may be readily determined. Moreover, should adjustments be deemed desirable, such adjustments may be made during the procedure and before the patient is sent to recovery.

[13] Another approach to treat mitral regurgitation with a device in the coronary sinus is based upon the observation that the application of a localized force against a discrete portion of the mitral valve annulus can terminate mitral regurgitation.

5 This suggests that mitral valve dilation may be localized and nonuniform. Hence, the device applies a force to one or more discrete portions of the atrial wall of the coronary sinus to provide localized mitral valve annulus reshaping instead of generalized reshaping of the mitral valve annulus. Such  
10 localized therapy would have all the benefits of the generalized therapy. In addition, a localized therapy device may be easier to implant and adjust.

[14] A still further approach to treat mitral regurgitation from the coronary sinus of the heart contemplates a device  
15 having a first anchor configured to be positioned within and fixed to the coronary sinus of the heart adjacent the mitral valve annulus within the heart, a cable fixed to the first anchor and extending proximally from the first anchor within the heart, a second anchor configured to be positioned in and fixed  
20 in the heart proximal to the first anchor and arranged to slidably receive the cable, and a lock that locks the cable on the second anchor. When the first and second anchors are fixed within the heart, the cable may be drawn proximally and locked on the second anchor. The geometry of the mitral valve is  
25 thereby effected. This approach provides flexibility in that the second anchor may be positioned and fixed in the coronary sinus or alternatively, the second anchor may be positioned and fixed in the right atrium. This approach further allows adjustments in the cable tension after implant. The present  
30 invention provides a still further alternative for treating mitral regurgitation with a device placed in the coronary sinus adjacent to the mitral valve annulus.

**SUMMARY OF THE INVENTION**

[15] The present invention provides a device that effects mitral valve annulus geometry of a heart. The device includes a first anchor configured to be positioned within and anchored to the coronary sinus of the heart adjacent the mitral valve annulus within the heart, and a second anchor configured to be positioned within the heart proximal to the first anchor and adjacent the mitral valve annulus within the heart. The device further includes a connecting member having a fixed length permanently attached to the first and second anchors. As a result, when the first and second anchors are within the heart with the first anchor anchored in the coronary sinus, the second anchor may be displaced proximally to effect the geometry of the mitral valve annulus and released to maintain the effect on the mitral valve geometry. The second anchor may be configured, when deployed, to anchor against distal movement but be moveable proximally to permit the second anchor to be displaced proximally within the coronary sinus.

[16] The first anchor and the second anchor are preferably self-deploying upon release in the coronary sinus or may be deployable after placement. Further, the connecting member, in being of fixed length, has a maximum extended length and as such may be a rigid member, have an initial arcuate configuration, include a spring, having a maximum length or be flexible but not stretchable.

[17] The present invention further provides a device for effecting mitral valve annulus geometry of a heart. The device includes first anchor means for anchoring in the coronary sinus of the heart adjacent the mitral valve annulus, and second anchor means for being deployed within the heart proximal to the first anchor means and adjacent the mitral valve annulus, and connecting means having a fixed length and permanently connecting the first anchor means to the second anchor means.



As a result, when the first and second anchor means are within the heart with the first anchor means anchored in the coronary sinus, the second anchor means may be displaced proximally for cooperating with the first anchor means and the connecting means for effecting the geometry of the mitral valve annulus and released for maintaining the effect on the mitral valve geometry.

**[18]** The invention further provides a system that effects mitral valve annulus geometry of a heart. The system includes a mitral valve device including a first anchor configured to be positioned within and anchored to the coronary sinus of the heart adjacent the mitral valve annulus within the heart, a second anchor configured to be positioned within the heart proximal to the first anchor and adjacent the mitral valve annulus within the heart, and a connecting member having a fixed length permanently attached to the first and second anchors.

**[19]** The system further includes a catheter having a distal end, a proximal end and a lumen that receives the device, the catheter being guidable into the coronary sinus adjacent to the mitral valve annulus and deploying the first and second anchors of the device within the coronary sinus adjacent to the mitral valve annulus, and a tether releasably coupled to the second anchor and extending proximally through the lumen and out of the catheter proximal end. As a result, when the first anchor is deployed by the catheter in the coronary sinus, the second anchor may be displaced proximally by proximally pulling on the tether to effect the geometry of the mitral valve annulus and thereafter released for deployment to maintain the effect on the mitral valve geometry.

**[20]** The present invention further provides a method of effecting mitral valve annulus geometry in a heart. The method includes the steps of fixing a first anchor within the coronary sinus of the heart adjacent to the mitral valve annulus,

positioning a second anchor within the coronary sinus adjacent to the mitral valve annulus and proximal to the first anchor, fixing a fixed length connecting member between the first anchor and the second anchor, displacing the second anchor proximally to effect the geometry of the mitral valve annulus, and releasing the second anchor from further proximal displacement to maintain the effect on the mitral valve geometry.

[21] The present invention further provides a device that effects mitral valve annulus geometry of a heart. The device includes a first anchor configured to be positioned within and anchored to the coronary sinus of the heart adjacent the mitral valve annulus within the heart, a second anchor configured to be positioned within the heart proximal to the first anchor and adjacent the mitral valve annulus within the heart, and a connecting member attached between the first and second anchors. At least one of the first and second anchors anchoring against movement in a first direction and being moveable in a second direction opposite the first direction.

[22] The at least one anchor may be the first anchor wherein the first direction is a proximal direction and wherein the second direction is a distal direction. The at least one anchor may be the second anchor wherein the first direction is a distal direction and wherein the second direction is a proximal direction. In a preferred embodiment, the first anchor anchors against movement in a proximal direction and is moveable in a distal direction and the second anchor anchors against movement in the distal direction and is moveable in the proximal direction.

[23] The invention still further provides a device that effects mitral valve annulus geometry of a heart and which permits a cardiac lead to be implanted in the left side of the heart. The device includes a first anchor configured to be positioned within and anchored to the coronary sinus of the

heart adjacent the mitral valve annulus within the heart, a second anchor configured to be positioned within the heart proximal to the first anchor and adjacent the mitral valve annulus within the heart, and a connecting member attached between the first and second anchors. The first anchor is configured to occupy less than all of the coronary sinus to permit a cardiac lead to be passed by the first anchor.

[24] The first anchor may include a loop through which the cardiac lead may be passed. The second anchor may be positionable within the coronary sinus and be configured to occupy less than all of the coronary sinus to permit the cardiac lead to be passed by the second anchor. The second anchor may also include a loop through which the cardiac lead may be passed.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[25] The features of the present invention which are believed to be novel are set forth with particularity in the appended claims. The invention, together with further aspects and advantages thereof, may best be understood by making reference to the following description taken in conjunction with the accompanying drawings, in the several figures of which like reference numerals identify identical elements, and wherein:

[26] **FIG. 1** is a superior view of a human heart with the atria removed;

[27] **FIG. 2** is a superior view of a human heart similar to **FIG. 1** illustrating a deployed mitral valve device embodying the present invention;

[28] **FIG. 3** is a superior view of a human heart similar to **FIG. 2** illustrating a first step in the deployment of the mitral valve device of **FIG. 2** embodying the present invention;

[29] **FIG. 4** is a view similar to **FIG. 3** illustrating a further step in the deployment of the device of **FIG. 2**;

[30] FIG. 5 is a view similar to FIG. 3 illustrating a final step in the deployment of the device of FIG. 2;

[31] FIG. 6 is a superior view of a human heart similar to FIG. 1 illustrating another deployed mitral valve device

5 embodying the present invention; and

[32] FIG. 7 is a side view with a portion broken away illustrating further details of device anchors and the manner in which they permit an implantable lead to pass thereby.

#### 10 DETAILED DESCRIPTION OF THE INVENTION

[33] Referring now to FIG. 1, it is a superior view of a human heart 10 with the atria removed to expose the mitral valve 12, the coronary sinus 14, the coronary artery 15, and the circumflex artery 17 of the heart 10 to lend a better  
15 understanding of the present invention. Also generally shown in FIG. 1 are the pulmonary valve 22, the aortic valve 24, and the tricuspid valve 26 of the heart 10.

[34] The mitral valve 12 includes an anterior cusp 16, a posterior cusp 18 and an annulus 20. The annulus encircles the  
20 cusps 16 and 18 and maintains their spacing to provide a complete closure during a left ventricular contraction. As is well known, the coronary sinus 14 partially encircles the mitral valve 12 adjacent to the mitral valve annulus 20. As is also known, the coronary sinus is part of the venous system of the  
25 heart and extends along the AV groove between the left atrium and the left ventricle. This places the coronary sinus essentially within the same plane as the mitral valve annulus making the coronary sinus available for placement of the mitral valve therapy device of the present invention therein.

30 [35] FIG. 2 shows a mitral valve therapy device 30 embodying the present invention. As may be noted in FIG. 2, the device 30 includes a first anchor 32, a connecting member 34, and a second anchor 36. The anchors 32 and 36 and the

connecting member 34 may be formed from the same material to provide an integral structure.

[36] The first anchor 32 is located at the distal end of the device 30. The anchor 32 is hook-shaped so as to be self-deployable when released in the coronary sinus 14. More specifically, the device 30 may be formed of most any biocompatible material such as stainless steel, Nitinol, a nickel/titanium alloy of the type well known in the art having shape memory or plastic. The hook-shaped configuration of the anchor 32 thus expands when released to wedge against the inner wall of the coronary sinus 14 for anchoring or fixing the anchor 32 against at least proximal movement. The anchor 32 may however allow distal movement. Preferably, the anchor 32 is positioned just proximally to the crossover point 19 of the coronary sinus 14 and a circumflex artery 17.

[37] The connecting member 34, by being formed of Nitinol, is relatively rigid and is predisposed to have an arcuate configuration to generally correspond to the shape of the mitral valve annulus 20. The connecting member 34 is of a fixed length and is permanently attached to the first and second anchors 32 and 36. Here it will be noted that the second anchor is positioned within the coronary sinus just distal to the ostium 21 of the coronary sinus 14. The second anchor 36 may have a similar hook-shaped configuration and is also preferably self-expanding to be self-deployable. The hook-shape of the anchor 36 anchors or fixes the anchor 36 against distal movement but permits the anchor to be pulled proximally. This is a particularly significant aspect of the device 30 because it permits the device to be adjusted after the anchors 32 and 36 are first deployed.

[38] When the device 30 is deployed as shown in FIG. 2, the first anchor 32 is fixed against proximal movement within the coronary sinus 14. The connecting member 34 then extends

proximally from the first anchor 32 to the second anchor 36. The second anchor 36 is then positioned in its desired location within the coronary sinus 14 proximal to the first anchor 32 and permitted to self-expand for being anchored against distal movement. Then, the second anchor 36 is pulled proximally while the first anchor 32 is held in its fixed position. This creates tension in the connecting member 34 to effect the geometry of the mitral valve annulus 20. Once a desired amount of tension is applied to the connecting member 34, the second anchor 36 is released from further movement and is redeployed against distal movement. With the connecting member 34 now under maintained tension, the advantageously effected geometry of the mitral valve annulus 20 is now preserved. The tension in the cable is preferably adjusted by the pulling on the second anchor 26 while monitoring a parameter indicative of mitral regurgitation, such as Doppler echo.

[39] The connecting member 34 may be provided with a covering (not shown). The covering may preferably be formed of a compressible material to serve to cushion the forces of the connecting member applied against the inner wall of the coronary sinus 14.

[40] FIGS. 3 through 5 show a manner in which the device 30 may be deployed by a deployment assembly 50. As will be noted in FIG. 3, the deployment assembly 50 includes a catheter 52 and a tether 54. The catheter 52 has a lumen 56 dimensioned for slidably receiving the device 30 in its predeployed state with the tether 54 looped around the second anchor 36 and extending out the proximal end of the catheter 52.

[41] As will be noted in FIG. 3, the first anchor 32 has been deployed while the second anchor remains in the catheter lumen 56. This may be accompanied by feeding the catheter 52 into the coronary sinus until the first anchor is in a desired position. Now, the catheter 52 may be moved proximally while

maintaining the first anchor 32 against movement. Proximal movement of the catheter 52 will release the anchor 32. When the anchor is released, it will self-expand to self-deploy and be fixed against proximal movement.

5    **[42]**       As shown in **FIG. 4**, the catheter 52 is further retracted to release the second anchor 36 to permit it to self-expand and to self-deploy. The second anchor 36 is now fixed against distal movement but permitted to move proximally. The tether 54 continues to extend out the proximal end of the  
10 catheter 52.

15    **[43]**       As may now be further seen in **FIG. 5**, tension is then applied to the connecting member 34 by proximally pulling on the tether 54, and hence the second anchor 36, while the first anchor 32 resists proximal movement. When the desired tension is placed on the connecting member 34, the second anchor 36 is released for re-self-deployment. When this is completed, the first anchor 32 and the second anchor 36 are fixed in position with a tension in the connecting member 34. The catheter 52 and the tether 54 may then be removed to complete the deployment  
20 process. Although the proximal anchor 36 is shown to be finally deployed in the coronary sinus, it will be appreciated by those skilled in the art that the proximal anchor 36, after being displaced proximally, may finally be deployed within the right atrium just proximal to the ostium 21 of the coronary sinus 14. Hence, any final position of the proximal anchor 36 proximal to  
25 the distal anchor 32 and within the heart is contemplated in accordance with the present invention.

30    **[44]**       In accordance with the present invention, the device 30 may be deployed in a slightly different manner as described above. Here, the first anchor 32 may be deployed as described above and the second anchor 36 left in the catheter 52 as it is moved proximally. When the second anchor 36 reaches a desired position, the catheter 52 may then be pulled back to release and

deploy the second anchor 36. As a result, in accordance with this alternative embodiment, the second anchor, when deployed, may anchor against both distal and proximal movement.

[45] FIG. 6 shows another mitral valve device 70 embodying the present invention. The device 70 is similar to the device 30 previously described except that its connecting member 74 includes a spring configuration 75. The spring 75 has a maximum length and serves to more forcefully maintain the applied tension on the mitral valve annulus 20. To this end, the device 70 includes a first anchor 72, the connecting member 74, and a second anchor 76.

[46] The first and second anchors 72 and 76 are again configured so that when they are released, they self-expand, to wedge against the inner wall of the coronary sinus 14. Again, the first anchor resists proximal movement and the second anchor 76 resists distal movement. In all other respects, the device 70 may be identical to and deployed in the same manner as the device 30.

[47] Implantable cardiac stimulation devices are well known in the art. Such devices may include, for example, implantable cardiac pacemakers and defibrillators. The devices are generally implanted in a pectoral region of the chest beneath the skin of a patient within what is known as a subcutaneous pocket. The implantable devices generally function in association with one or more electrode carrying leads which are implanted within the heart. The electrodes are usually positioned within the right side of the heart, either within the right ventricle or right atrium, or both, for making electrical contact with their respective heart chamber. Conductors within the leads and a proximal connector carried by the leads couple the electrodes to the device to enable the device to sense cardiac electrical activity and deliver the desired therapy.



[48] Traditionally, therapy delivery had been limited to the venous, or right side of the heart. The reason for this is that implanted electrodes can cause blood clot formation in some patients. If a blood clot were released arterially from the left heart, as for example the left ventricle, it could pass directly to the brain potentially resulting in a paralyzing or fatal stroke. However, a blood clot released from the right heart, as from the right ventricle, would pass into the lungs where the filtering action of the lungs would prevent a fatal or debilitating embolism in the brain.

[49] Recently, new lead structures and methods have been proposed and even practiced for delivering cardiac rhythm management therapy to the left heart. These lead structures and methods avoid direct electrode placement within the left atrium and left ventricle of the heart by lead implantation within the coronary sinus of the heart. As previously mentioned, the phrase "coronary sinus" refers to not only the coronary sinus itself but in addition, the venous system associated with the coronary sinus including the great cardiac vein.

[50] It has been demonstrated that electrodes placed in the coronary sinus region of the heart may be used for left atrial pacing, left ventricular pacing, or cardioversion and defibrillation. These advancements enable implantable cardiac stimulation devices to address the needs of a patient population with left ventricular dysfunction and/or congestive heart failure which would benefit from left heart side pacing, either alone or in conjunction with right heart side pacing (bi-chamber pacing), and/or defibrillation.

[51] Even though the device of the present invention is implantable in the coronary sinus of the heart, it is configured in accordance with further aspects of the present invention to permit a cardiac lead to pass through the coronary sinus for functioning as described above. To that end, and as best seen

in FIG. 7, the anchors 32 and 36 of the device 30 occupy only a small portion of and hence less than all of the interior space of the coronary sinus 14. This permits a cardiac lead 80 to be advanced into the coronary sinus 14 for implant in the left side  
5 of the heart.

[52] More specifically, the anchors 32 and 36 take the form of loops 33 and 35 respectively which are then bent backwards on the device to form the previously referred to hook-shapes for self-deployment. The loops 33 and 35 thus permit the cardiac  
10 lead 80 to be passed therethrough for implant in the left heart. This is particularly desirable because many patients suffering from mitral regurgitation may also be candidates for left heart cardiac rhythm management therapy.

[53] While particular embodiments of the present invention  
15 have been shown and described, modifications may be made, and it is therefore intended in the appended claims to cover all such changes and modifications which fall within the true spirit and scope of the invention as defined by the appended claims.

What is claimed:

1. A device that effects mitral valve annulus geometry of a heart, comprising:

5       a first anchor configured to be positioned within and anchored to the coronary sinus of the heart adjacent the mitral valve annulus within the heart;

          a second anchor configured to be positioned within the heart proximal to the first anchor and adjacent the mitral  
10       valve annulus within the heart; and

          a connecting member having a fixed length permanently attached to the first and second anchors, whereby

          when the first and second anchors are within the heart with the first anchor anchored in the coronary sinus, the  
15       second anchor may be displaced proximally to effect the geometry of the mitral valve annulus and released to maintain the effect on the mitral valve geometry.

2. The device of claim 1 wherein the second anchor, when deployed, is configured to anchor against distal movement and  
20       moveable in a proximal direction.

3. The device of claim 2 wherein the first anchor is self-deploying upon release in the coronary sinus.

4. The device of claim 2 wherein the second anchor is self-deploying upon release in the coronary sinus.

25       5. The device of claim 2 wherein the connecting member is a rigid member.

6. The device of claim 2 wherein the connecting member includes a spring having a maximum length.

7. The device of claim 2 wherein the connecting member is  
30       flexible and nonstretchable.

8. A device for effecting mitral valve annulus geometry of a heart, comprising:

first anchor means for anchoring in the coronary sinus of the heart adjacent the mitral valve annulus;

second anchor means for being deployed within the heart proximal to the first anchor means and adjacent the mitral valve annulus; and

connecting means having a fixed length and permanently connecting the first anchor means to the second anchor means, whereby

when the first and second anchor means are within the heart with the first anchor means deployed, the second anchor means may be displaced proximally for cooperating with the first anchor means and the connecting means for effecting the geometry of the mitral valve annulus and released for maintaining the effect on the mitral valve geometry.

9. The device of claim 8 wherein the second anchor means, when deployed, anchors against distal movement and is moveable in a proximal direction.

10. The device of claim 8 wherein the first anchor means is self-deploying upon release in the coronary sinus.

11. The device of claim 8 wherein the second anchor means is self-deploying upon release in the coronary sinus.

12. The device of claim 8 wherein the connecting means is a rigid member.

13. The device of claim 8 wherein the connecting means includes a spring having a maximum length.

14. The device of claim 8 wherein the connecting means is flexible and nonstretchable.

15. The device of claim 1 wherein the first anchor occupies less than all of the coronary sinus to permit a cardiac lead to be passed by the first anchor.

16. The device of claim 15 wherein the first anchor includes a loop through which the cardiac lead may be passed.

17. The device of claim 15 wherein the second anchor also occupies less than all of the coronary sinus to permit the cardiac lead to be passed by the second anchor.

18. The device of claim 17 wherein the second anchor  
5 includes a loop through which the cardiac lead may be passed.

19. A system that effects mitral valve annulus geometry of a heart, comprising:

a mitral valve device including a first anchor  
configured to be positioned within and anchored to the  
10 coronary sinus of the heart adjacent the mitral valve annulus within the heart, a second anchor configured to be positioned within the heart proximal to the first anchor and adjacent the mitral valve annulus within the heart, and a connecting member having a fixed length permanently  
15 attached to the first and second anchors;

a catheter having a distal end, a proximal end and a lumen that receives the device, the catheter being guidable into the coronary sinus adjacent to the mitral valve annulus and deploying the first and second anchors of the  
20 device within the coronary sinus adjacent to the mitral valve annulus; and

a tether releasably coupled to the second anchor and extending proximally through the lumen and out of the catheter proximal end, whereby

25 when the first anchor is deployed by the catheter in the coronary sinus, the second anchor may be displaced proximally by proximally pulling on the tether to effect the geometry of the mitral valve annulus and thereafter released for deployment to maintain the effect on the  
30 mitral valve geometry.

20. The system of claim 19 wherein the second anchor, when deployed, is anchored against distal movement and moveable in a proximal direction.

21. The system of claim 19 wherein the first anchor is self-deploying upon release in the coronary sinus.

22. The system of claim 19 wherein the second anchor is self-deploying upon release in the coronary sinus.

5 23. The system of claim 19 wherein the connecting member is a rigid member.

24. The system of claim 19 wherein the connecting member includes a spring having a maximum length.

10 25. The system of claim 19 wherein the connecting member is flexible and nonstretchable.

26. A method of effecting mitral valve annulus geometry in a heart, the method including the steps of:

fixing a first anchor within the coronary sinus of the heart adjacent to the mitral valve annulus;

15 positioning a second anchor within the heart proximal to the first anchor;

fixing a fixed length connecting member between the first anchor and the second anchor;

20 displacing the second anchor proximally to effect the geometry of the mitral valve annulus; and

releasing the second anchor from further proximal displacement to maintain the effect on the mitral valve geometry.

25 27. The method of claim 26 wherein the displacing step includes the steps of releasably coupling a tether to the second anchor and pulling proximally on the tether.

28. The method of claim 27 including the further step of removing the tether from the second anchor after the releasing step.

30 29. A method of effecting mitral valve geometry of a heart, the method including the steps of:

advancing a guide catheter into the coronary sinus of the heart adjacent to the mitral valve annulus;

feeding a self-deploying first anchor down and out of the guide catheter to deploy the first anchor in the coronary sinus adjacent to the mitral valve annulus;

connecting a fixed length connecting member between the first anchor and a self-deploying second anchor that once deployed anchors at least against distal movement;

guiding the second self-deploying anchor down the guide catheter to a position within the coronary sinus proximal to the first anchor;

displacing the second anchor proximally to effect the geometry of the mitral valve annulus;

withdrawing the guide catheter to release and deploy the second anchor; and

releasing the second anchor to deploy the second anchor and maintain the effect on the mitral valve annulus geometry.

30. The method of claim 29 including the further step of releasably coupling a tether to the second anchor prior to the displacing step.

31. The method of claim 30 wherein the displacing step includes the step of pulling proximally on the tether.

32. The method of claim 29 wherein the feeding step includes locating the first anchor proximally to the circumflex artery within the coronary sinus.

33. A device that effects mitral valve annulus geometry of a heart, comprising:

a first anchor configured to be positioned within and anchored to the coronary sinus of the heart adjacent the mitral valve annulus within the heart;

a second anchor configured to be positioned within the heart proximal to the first anchor and adjacent the mitral valve annulus within the heart; and

a connecting member attached between the first and second anchors,

at least one of the first and second anchors anchoring against movement in a first direction and being moveable in a second direction opposite the first direction.

34. The device of claim 33 wherein the at least one anchor is the first anchor wherein the first direction is a proximal direction and wherein the second direction is a distal direction.

35. The device of claim 33 wherein the at least one anchor is the second anchor wherein the first direction is a distal direction and wherein the second direction is a proximal direction.

36. The device of claim 33 wherein the first anchor anchors against movement in a proximal direction and is moveable in a distal direction and wherein the second anchor anchors against movement in the distal direction and is moveable in the proximal direction.

37. A device that effects mitral valve annulus geometry of a heart, comprising:

a first anchor configured to be positioned within and anchored to the coronary sinus of the heart adjacent the mitral valve annulus within the heart;

a second anchor configured to be positioned within the heart proximal to the first anchor and adjacent the mitral valve annulus within the heart; and

a connecting member attached between the first and second anchors,

the first anchor being configured to occupy less than all of the coronary sinus to permit a cardiac lead to be passed by the first anchor.

38. The device of claim 37 wherein the first anchor includes a loop through which the cardiac lead may be passed.



39. The device of claim 37 wherein the second anchor is positionable within the coronary sinus and wherein the second anchor is configured to occupy less than all of the coronary sinus to permit the cardiac lead to be passed by the second anchor.

40. The device of claim 39 wherein the second anchor includes a loop through which the cardiac lead may be passed.

41. The device of claim 39 wherein each of the first and second anchors includes a loop through which the cardiac lead may be passed.

42. The device of claim 1 wherein the connecting member is flexible and nonstretchable.

43. A device for providing therapy to a mitral valve annulus of a heart, the device being elongated and dimensioned to be received within the coronary sinus of the heart adjacent to the mitral valve annulus, the device having a first radius of curvature when initially placed in the coronary sinus adjacent the mitral valve annulus and a second radius of curvature when providing therapy to the mitral valve annulus from within the coronary sinus, the second radius of curvature being greater than the first radius of curvature.

1/4

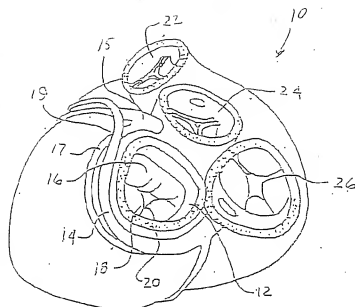


FIG. 1

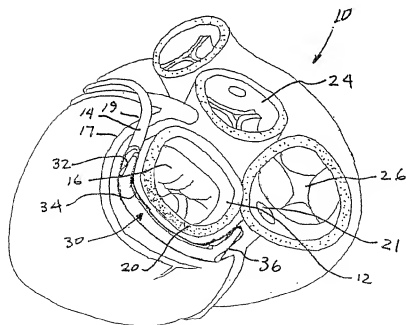


FIG. 2

2/4

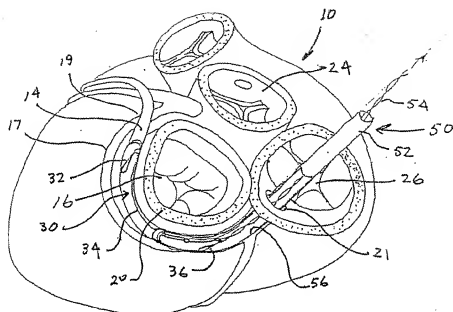


FIG. 3

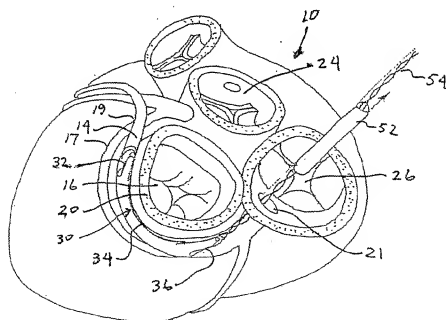


FIG. 4

3/4

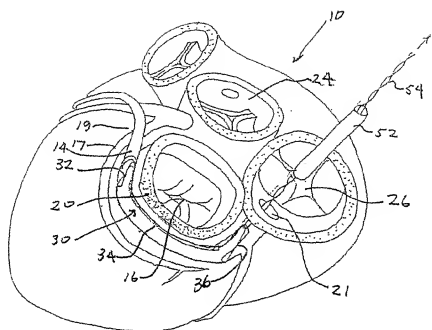


FIG. 5

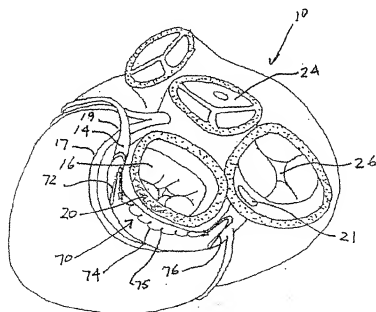


FIG. 6

4/4

